





# Sani-lok® Barrier Adapter Connection Configurations for Different Reprocessing Equipment

Renatron & Renatron II Connections  
(either configuration may be in use)

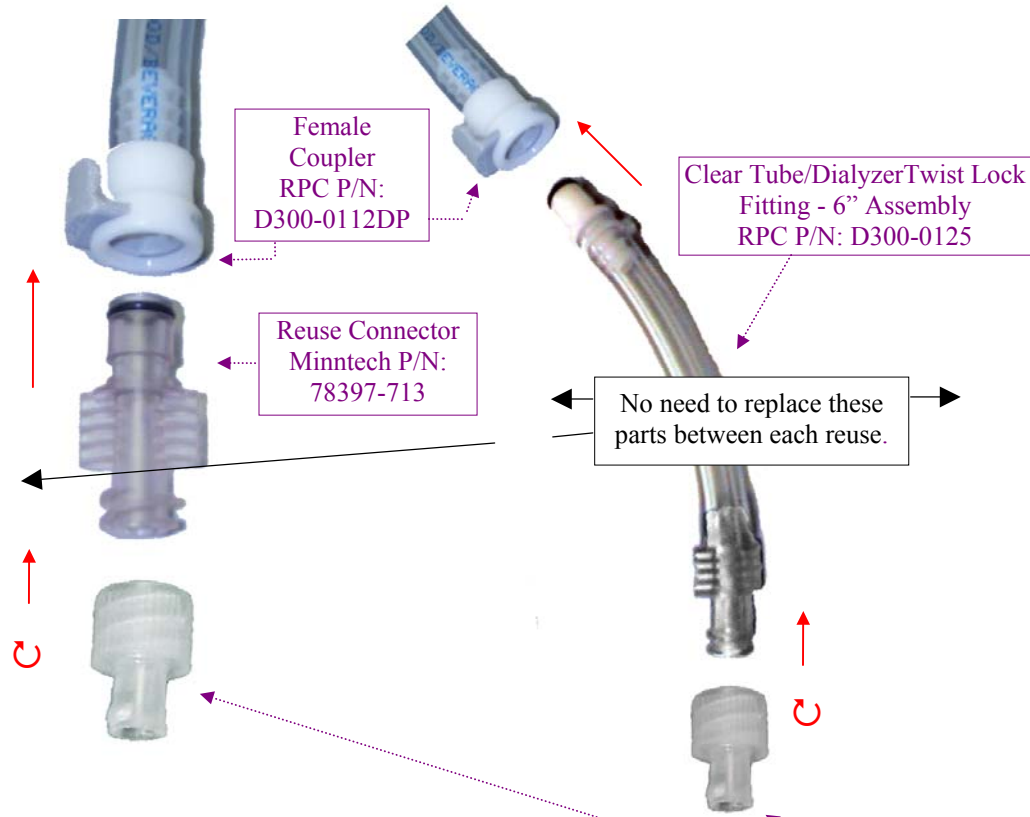

DRS-4 Connection

Echo & Manual System Connection

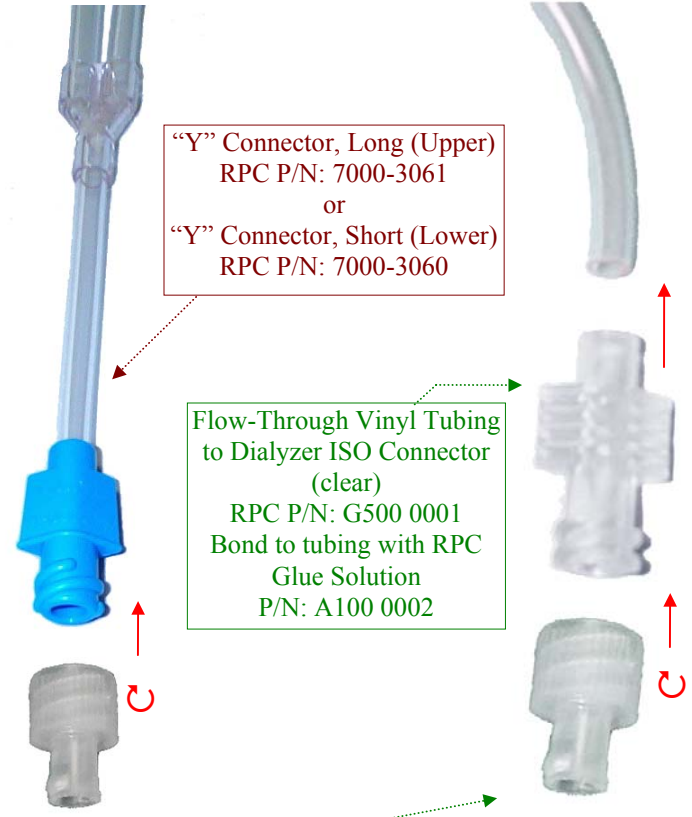

**Sani-lok® Barrier Adapter - RPC Part Number 7000-1050**  
**See RPC Instructions/Application Note Number 00303**

Important Note: Calibrate reuse equipment using manufacturers instructions.  
Calibration procedure is typically performed with all connectors in place.

Sani-lok is a registered trademark of RPC  
Renatron/II is a trademark of Minntech Corp.  
DRS-4 is a trademark of Fresenius Medical  
Echo is a trademark of Mesa Laboratories